



**User's Manual**

# **GTCDx™ Anti-AAV2 antibody ELISA Kit**



**DEIASL347**



**96T**





This product is for research use only and is not intended for diagnostic use.

For illustrative purposes only. To perform the assay the instructions for use provided with the kit have to be used.

---

**Creative Diagnostics**

 **Address: 45-1 Ramsey Road, Shirley, NY 11967, USA**

 **Tel: 1-631-624-4882 (USA) 44-161-818-6441 (Europe)**  **Fax: 1-631-938-8221**

 **Email: [info@creative-diagnostics.com](mailto:info@creative-diagnostics.com)**  **Web: [www.creative-diagnostics.com](http://www.creative-diagnostics.com)**

---

## PRODUCT INFORMATION

### Intended Use

The Anti-AAV2 ELISA is used as an analytical tool for qualitative determination of antibodies to AAV2 in serum.

### General Description

Researchers have used AAV-based vectors in pre-clinical research and in clinical trials in which AAV-based vectors have demonstrated a good safety profile. AAVs have also demonstrated lasting therapeutic gene expression following a single treatment in preclinical and clinical studies.

Recombinant vectors based on AAV2 (rAAV2) have been, or are currently being, used in a number of Phase I/II clinical trials, and thus far, no serious adverse events, much less cancer of any type have ever been observed or reported. Furthermore, the use of rAAV2 vectors has led to clinical efficacy in the potential gene therapy of at least three human diseases: Leber's congenital amaurosis (LCA), aromatic L-amino acid decarboxylase deficiency (AADC) and choroideremia.

One of the major challenges in AAV-based gene therapy is the presence of circulating anti-AAV neutralizing antibodies, which can pre-exist in patients and may prevent successful gene transfer. High levels of circulating anti-AAV neutralizing antibodies can develop after a single administration of gene therapy and can prevent successful gene transfer in patients.

### Principles of Testing

The qualitative immunoenzymatic determination of specific antibodies is based on the ELISA (Enzyme-linked Immunosorbent Assay) technique.

AAV2 capsid protein is precoated onto microwells. Samples and control are pipetted into microwells and antibodies to AAV2 present in the sample are bound by the capture protein. After incubation, washing is done to remove the unbound Anti-AAV2. An enzyme linked polyclonal antibody specific for human IgG is pipetted and incubated. After washing microwells in order to remove any non-specific binding, the ready to use substrate solution (TMB) is added to microwells and color develops proportionally to the amount of antibodies to AAV2 in the sample. Color development is then stopped by addition of stop solution. Absorbance at 450/620 nm is read using an ELISA Microtiterplate reader.

### Reagents And Materials Provided

1. AAV2 Capsid Coated Microtiter Plate, 12 × 8 wells
2. Negative Control, ready to use, 1 × 1 ml
3. Anti-AAV2 Positive Control, ready to use, 1 × 1 ml
4. Cut-off Control, ready to use, 1 × 1 ml
5. Anti-human IgG Conjugate, ready to use, 1 × 12 ml
6. Sample Diluent, ready to use, 1 × 50 ml
7. Wash Buffer, 20 × concentrate, 1 × 50 ml

8. TMB Substrate, ready to use, 2 × 6 ml
9. Stop Solution, ready to use, 1 × 7 ml
10. Instruction Manual

## Materials Required But Not Supplied

1. Microtiter Plate Reader able to measure absorbance at 450 nm, with the correction wavelength set at 620 nm
2. Adjustable pipettes and multichannel pipettor to measure volumes ranging from 25 ul to 1000 ul
3. Deionized (DI) water
4. Wash bottle or automated microplate washer
5. Graph paper or software for data analysis
6. Timer
7. Absorbent Paper

## Storage

1. All reagents should be stored at 2°C to 8°C for stability.
2. All reagents and wash buffer should be used within 12 months from manufacturing date.
3. Before using, bring all components to room temperature (18-25°C). Upon assay completion ensure all components of the kit are returned to appropriate storage conditions.
4. The Substrate is light-sensitive and should be protected from direct sunlight or UV sources.

## Specimen Collection And Preparation

### 1. Serum

Use a serum separator tube (SST) and allow samples to clot for 30 minutes at room temperature before centrifugation for 10-15 minutes at 1500 × g. Remove serum and assay immediately or aliquot and store samples at ≤ -20°C. Avoid repeated freeze-thaw cycles. **Note: Lipaemic, hemolytic or contaminated samples should not be run.**

### Sample Preparation Before Use

Allow samples to reach room temperature prior to assay. Take care to agitate patient samples gently in order to ensure homogeneity.

Samples have to be diluted 1 in 50 (v/v), e.g. 10 ul sample in 490 ul sample diluent, prior to assay. The samples may be kept at 2 - 8°C for up to three days. Long-term storage requires -20°C.

## Plate Preparation

	1	2	3	4	5	6	7	8	9	10	11	12
A	N.C.		S6		S14		S22		S30		S38	
B	C.O.		S7		S15		S23		S31		S39	
C	P.C.		S8		S16		S24		S32		S40	
D	S1		S9		S17		S25		S33		S41	
E	S2		S10		S18		S26		S34		S42	
F	S3		S11		S19		S27		S35		S43	
G	S4		S12		S20		S28		S36		S44	
H	S5		S13		S21		S29		S37		S45	

\* All controls and samples are run in duplicates

P.C. – Positive control

C.O. – Cut-off control

N.C. – Negative control

S. – Sample

## Reagent Preparation

1. Label any aliquots made with the kit Lot No. and Expiration date and store it at appropriate conditions mentioned.
2. Bring all reagents to Room temperature before use.
3. To make Wash Buffer (1x): dilute 50 ml of 20x Wash Buffer in 950 ml of DI water.

## Assay Procedure

### Procedural Notes:

1. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess un-reacted reagents is essential.
2. High Dose Hook Effect may be observed in samples with very high concentrations of Anti-AAV2. High Dose Hook Effect is due to excess of antibody for very high concentrations of Anti-AAV2 present in the sample. High Dose Hook effect is most likely encountered from samples early in the purification process. If Hook Effect is possible, the samples to be assayed should be diluted with a compatible diluent. Thus if the Anti-AAV2 concentration of the undiluted sample is less than the diluted sample, this may be indicative of the Hook Effect.
3. Avoid assay of Samples containing Sodium Azide ( $\text{NaN}_3$ ), as it could destroy the HRP activity resulting in under-estimation of the amount of Anti-AAV2.
4. It is recommended that all Controls and Samples be assayed in duplicates.
5. Maintain a repetitive timing sequence from well to well for all the steps to ensure that the incubation timings are same for each well.
6. If the Substrate has a distinct blue color prior to use it may have been contaminated and use of such substrate can lead to compromisation of the sensitivity of the assay.
7. The plates should be read within 30 minutes after adding the Stop Solution.
8. Make a work list in order to identify the location of Controls and Samples.

### Assay Steps:

1. It is strongly recommended that all Controls and Samples be run in duplicates or triplicates. All steps must

be performed at 37°C.

2. Add 100 ul of Anti-AAV2 Positive Control, Cut-off Control, Negative Control, and diluted Samples into respective wells.
3. Cover the plate and incubate for 30 minutes at 37°C.
4. Aspirate and wash plate 5 times with Wash Buffer (1x) and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step.
5. Pipette without delay in the same order 100 ul of Anti-human IgG Conjugate into each well.
6. Cover the plate and incubate for 30 minutes at 37°C.
7. Aspirate and wash plate 5 times with Wash Buffer (1x) and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step.
8. Add 100 ul of TMB Substrate in each well.
9. Incubate the plate for 15 minutes at 37°C in dark. Positive wells should turn bluish in color. (**DO NOT SHAKE** or else it may result in higher backgrounds and worse precision).
10. Pipette out 50 ul of Stop Solution. Wells should turn from blue to yellow in color.
11. Measure the absorbance at 450/620 nm within 30 min after addition of the Stop Solution.

## Calculation

Determine the Mean Absorbance for each set of duplicate control and Samples.

Calculate average (Avg) OD: Avg OD = Average OD from AAV2 Capsid Coated Microtiter Plate

## Quality Control

It is recommended that for each laboratory assay appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

For a valid assay, Negative Control, Cut-off Control, and Positive Control should fall in the Avg O.D. values below.

Control Result for Valid Assay	Calculated Avg O.D. Values
Negative Control	<0.1
Cut-off Control	0.1-0.5
Positive Control	>cut-off

## Results in Units [U]

Avg OD/Cut-off= [Units = U]

Example: 1.591/0.43=3.7 U (Units)

## Interpretation Of Results

<b>Cut-off</b>	<b>1 U</b>	
<b>Positive</b>	<b>&gt;1.1 U</b>	<b>aav2 IgG antibody detected</b>
<b>Equivocal</b>	<b>0.9-1.1 U</b>	<b>Repeat the test. If sample gives a similar O.D., then aav2 IgG antibody cannot be determined, and testing should be repeated by an alternative method or another sample should be collected</b>
<b>Negative</b>	<b>&lt;0.9 U</b>	<b>No detectable aav2 IgG antibody</b>

## Reference Values


The levels of the Anti-AAV2 antibodies (IgG) were analysed with this ELISA in a panel of 76 healthy blood donors. With a cut-off of 1 U, 76% of the blood donors were Anti-AAV2 positive (IgG) which reflects the known percentage of infections in the general population.

	<b>No.of samples</b>	<b>Percentage</b>
<b>Positive</b>	<b>58</b>	<b>76.3%</b>
<b>Equivocal</b>	<b>3</b>	<b>3.9%</b>
<b>Negative</b>	<b>15</b>	<b>19.7%</b>

## Performance Characteristics

### Function verification

Non-scaled Venn diagram depicting the relationship between total (tAb) and specific confirmed total antibodies in samples. The results are highly consistent, indicating that ELISA has high accuracy in detecting AAV antibodies.

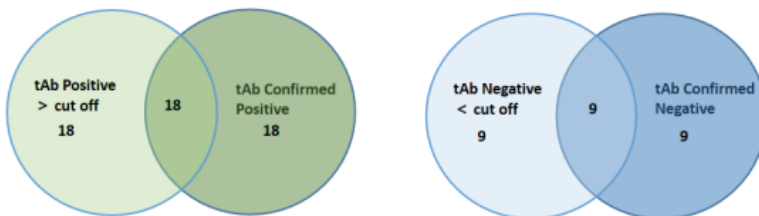

## Precision

<b>Intra-Assay</b>		
<b>Sample</b>	<b>Mean</b>	<b>CV(%)</b>
<b>1</b>	<b>0.325</b>	<b>5%</b>
<b>2</b>	<b>0.762</b>	<b>3%</b>
<b>3</b>	<b>1.524</b>	<b>3%</b>

<b>Inter-Assay</b>		
<b>Sample</b>	<b>Mean</b>	<b>CV(%)</b>
<b>1</b>	<b>0.368</b>	<b>5%</b>
<b>2</b>	<b>0.815</b>	<b>5%</b>
<b>3</b>	<b>1.422</b>	<b>6%</b>

## Precautions

1. This Kit is For Research Use only. Follow the working instructions carefully.
2. The expiration dates stated on the kit are to be observed. The same relates to the stability stated for reconstituted reagents.
3. Do not use or mix reagents from different lots.

4. Do not use reagents from other manufacturers.
5. Avoid time shift during pipetting of reagents.
6. All reagents should be kept at 2 - 8 °C before use in the original shipping container.
7. Source materials maybe derived from human body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
8. Since the kit contains potentially hazardous materials, the following precautions should be observed
  - Do not smoke, eat or drink while handling kit material
  - Always use protective gloves
  - Never pipette material by mouth
  - Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
9. In any case GLP should be applied with all general and individual regulations to the use of this kit.